



Basic contact lens course

Part 7 - RGP lens selection

Andy Franklin and **Ngairé Franklin** describe how to select the initial lens for a rigid gas-permeable (RGP) fitting and how to calculate the final order. **Module C14190**, suitable as one general point for optometrists and dispensing opticians, one specialist point for CLOs



Choosing the back optic zone radius (BOZR)

The intended relationship between the cornea and the back optic zone of the lens will depend on the fitting philosophy adopted. The lens is held in place on the cornea both by the eyelids and by surface tension, which act at the lens edge where it is not covered by the lid. If the edge clearance is excessive no meniscus forms and no surface tension acts. Reduced edge clearance and edge thickness boosts surface tension. Broadly speaking, there are two extreme positions that can be adopted.

● **Lid attachment** ('big and flat'). Here we may have a lens of about 9.50mm diameter, a back optic zone diameter (BOZD) of about 8.40mm and a BOZR 0.2-0.3 flatter than K. It needs to be this flat with a BOZD this size in order to be flatter than alignment with the cornea. Essentially, the centration and movement of the lens is controlled by the lids, which pass the lens between upper and lower during the blink cycle. Lenses fitted like this do have a habit of riding a little high, especially in the long term, and exposure stain of the lower cornea is common

● **Interpalpebral** ('small and steep'). The lens is fitted with a small total diameter (TD) (typically around 8.5mm) and BOZD to minimise lid interference. Generally the BOZR is fitted to give some apical clearance, and this was often done by adding 25-30 per cent of the corneal toricity to the flattest K, a procedure which has unfortunately persisted into 'alignment' fitting, where it is inappropriate. Interpalpebral fits are often rather uncomfortable, due to the interaction of lens edge and lid margins.

Most lenses these days are fitted for an 'alignment' fit that is some way between the two extremes. It

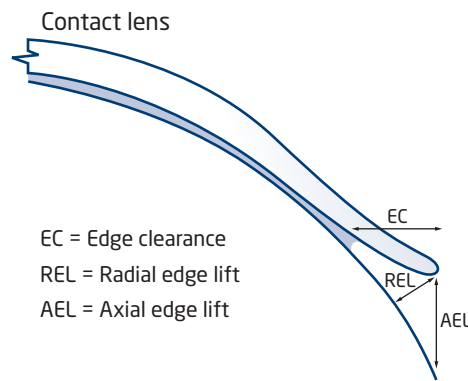


Figure 1
Axial and radial edge lift and edge clearance

should be emphasised that there isn't just one way of fitting lenses, and the short history of rigid lenses contains examples of very flat and very steep (0.3mm in the Bayshore method) lenses by modern standards, which seemed to work well at least on some patients. If the standard alignment fit doesn't work another philosophy might, so never be afraid to try something different.

Alignment fitting

The idea here is to fit the back optic zone in close alignment with the front surface of the cornea, with a uniform, thin tear film between the two. This is a goal rather than something that is actually perfectly realised, but perfect alignment probably wouldn't work very well. The advantages of an alignment fit are as follows.

● The weight of the lens, and the force translated through the lens during the blink cycle is spread over the maximum area. If either is too localised, corneal warpage can occur

● Lens flexure is minimised, which will ensure good visual performance and minimise mechanical stress on the cornea. This is quite an important

consideration when using modern high-Dk RGP lenses

● Provided that the periphery of the lens is also well designed, the thin tear film under the central part of the lens will be easily replenished with oxygen and never become stagnant. Furthermore, a thin tear film will not produce a major 'barrier effect', slowing the movement of oxygen through the lens to the cornea. A thicker tear film could produce the situation where the rate of flow of oxygen allowed through the tear film is less than the rate that the lens itself is capable of. Barrier effects reduce the oxygen transmission of all RGPs, especially those with high Dks.

It should be remembered that K readings are taken at points not far away from the corneal apex, whereas we are trying to align an area of cornea over twice as wide. For the majority of patients the spherical curve that will best align with the cornea will be somewhat flatter than K, and the wider the BOZD, the flatter we need to go. In practice, fitting on flattest K seems to work well with conventional designs of 9.00mm diameter or thereabouts. Once we get up to 9.50mm, we need to go flatter, because the average corneal radius is likely to be flatter. On a larger diameter, the primary sag of a spherical curve increases, resulting in a steeper-fitting lens. Therefore, if you increase the BOZD by 0.5mm, you need to flatten the BOZR by 0.05mm to achieve a 'clinically equivalent fit'.

Most lenses fitted on flattest K are probably a fraction steeper than alignment really, but this seems to work well and may aid centration without seriously compromising in other respects. With an alignment fit, the practice of steepening the BZOR by a proportion of the corneal toricity is



inappropriate as any steepening of the fit along the flattest meridian will only serve to push the whole lens further from the cornea, inducing central clearance. It will therefore have no effect on edge stand-off in the steeper meridian which is the usual intention. It does sometimes help the lens to centre though, if a back surface toric is not an attractive option.

If you are fitting an aspheric design, it's probably best to read the manufacturer's recommendations as the nominal BOZR initially selected will be related to the degree of asphericity ('eccentricity' or 'shape factor') of the lens design. The principles are similar though.

The periphery

The periphery of the lens may be generated either by working a set (typically 3 or 4) of progressively flatter spherical curves on to the back surface, or as a consequence of using an aspheric curve. In either case, it is worth considering what we have a periphery for. Part of the reason has to do with tear circulation under the lens. If we don't have edge clearance tear fluid will not be able to get under the lens. This will have two effects. Firstly the lubricative effect of the tear film would be lost. The lens is then likely to adhere to the epithelium and eventually mechanical damage to this vital layer will occur. Secondly, the oxygen normally carried by the circulating tears will be lost to the cornea under the lens. This is not too important provided the lens is able to transmit sufficient oxygen through its own substance, but for a lens of low transmission, tear exchange may be an important source of oxygen delivery. Central corneal hypoxia will compromise epithelial integrity further. Clearly then we must have enough peripheral clearance to allow

TABLE 1
Minimum centre thickness recommended for low minus lenses

Lens power (D)	Centre thickness (mm)
-1.00	0.18
-2.00	0.17
-3.00	0.16
-4.00	0.15
-5.00 and over	0.14

adequate tear exchange.

The other reason for peripheral clearance became apparent when silicone acrylate lenses first appeared. Practitioners reasoned that improved oxygen transmission reduced the need for tear exchange, and lenses with very little edge clearance were both more comfortable and tended to centre well, due to the improved tear meniscus around the lens.

The downside to all this became apparent when it was time to remove the lenses, as a certain amount of edge clearance is needed to allow the eyelids to dislodge the lens. The problem was made slightly worse by the fact that many of the patients being fitted with these lenses were used to PMMA lenses, which needed quite a lot of edge clearance in order to get oxygen to the cornea. Removal techniques made sloppy by loosely fitting lenses (a sharp tap to the back of the head would probably have removed some of the designs then in common use) were severely challenged by the minimal peripheries of the RGPs. A tactical withdrawal to slightly more generous peripheries was undertaken.

Modern 'system' lenses have peripheries that are worked out by computer to give a smooth progression and where spherical curves are used the transitions between them are

polished to 'blend' the curves into one continuous surface. They are calculated to work on the majority of patients, but if a patient has an unusual corneal shape factor too much or too little edge clearance will result. This can be detected once the lens is observed on the eye with fluorescein, and laboratories can increase or decrease the edge lift of the lens produced while keeping the optic zone the same. For a lens ordered empirically, a system lens is usually the best bet, unless you are aware of unusual corneal characteristics.

The terms edge clearance and edge lift are not interchangeable. Edge clearance refers to the gap between the front surface of the cornea and the back surface of the peripheral curves, and it is edge clearance that is observable with fluorescein. Edge lift is a geometrical characteristic of the lens itself, and is definable in either axial or radial forms. The difference between them is shown in Figure 1.

Edge profile

The shape of the edge is an important determinant of lens comfort, especially in the early stages. Laboratories tend to have their standard designs, but if you find that the lenses coming through are not as comfortable as they should be, you could ask for a different form (or change labs, of course). Generally, for the alignment fit with partial lid attachment it is interaction between the lens edge and the eyelids rather than the cornea that seems to determine comfort. Rounding of the anterior rather than the posterior edge seems to be the important factor.

Centre thickness

Modern lenses, because of their material properties and thin design, tend to flex, especially in low minus-powered lenses. In general, flexure increases with Dk, and with the degree of toricity of



Maura Burnett BSc (Hons) MCOptom. One of a team of 15 Practice Academy consultants

Practice ACADEMY

BRINGING THE ACADEMY
FOR EYECARE EXCELLENCE™
TO YOUR PRACTICE.

Contact your CIBA VISION Business Development Manager and find out how your practice can benefit from high quality, **in-store** training delivered by a Practice Academy consultant



"The training was brilliant. We haven't had training to this depth before. It boosted our knowledge of multifocal contact lenses and our confidence in offering multifocal contact lenses, even to the early presbyopes."

Claire Burnell, Assistant Practice Manager, D&A Opticians, West Wickham



CET Contact Lens Monthly

the cornea the lens is sitting on. The minimum thickness desirable for a given power is shown in Table 1. In general, 'system' lenses take care of this for you. Once corneal astigmatism gets to about 2.00D a further 0.02mm is needed, so if you are fitting an astigmatic cornea with a spherical lens you might need to order something a bit thicker. This will, of course, compromise the oxygen transmission a little.

Back vertex power

The power of the contact lens required would normally be calculated from the spectacle prescription corrected for vertex distance, but must take the power of the tear lens between the contact lens and cornea into consideration. If the lens is in perfect alignment with the central cornea, it follows that the tear lens will have zero dioptric power, and over-refraction is rather a good way to measure the degree of alignment. A lens which is steeper than the cornea will give rise to a tear lens of positive power, and a flat lens will create a negative tear lens. The power of the tear lens can be calculated precisely, but for lenses fitted fairly close to alignment this is unnecessary. A simple rule of thumb exists. For every 0.05mm that the BOZR is steeper than K, the tear lens power increases by +0.25D. Therefore you must counter this by adding -0.25D to the power of the contact lens. Obviously if the contact lens is flat by 0.05mm, an extra -0.25 is added to the power of the tear lens, and the power of the lens ordered must be increased by +0.25D.

Example

A patient has a spectacle prescription of -5.00 DS at a back vertex distance of 10mm. His K readings are 7.80mm in all meridians, but we have elected to fit him with a lens with a BOZD of 7.75mm.

The first step is to adjust the spectacle lens power to account for the fact that the contact lens is sitting on the eye. This can be calculated using the formula:

$$L = \frac{F's}{1-dF's}$$

Where L = power of contact lens
d = vertex distance of spec lens
F's = power of spectacle lens

However, it's much easier to look it up in a table, such as that provided in the Association of Contact Lens Manufacturers' manual. A spectacle lens at 10mm BVD has an effective

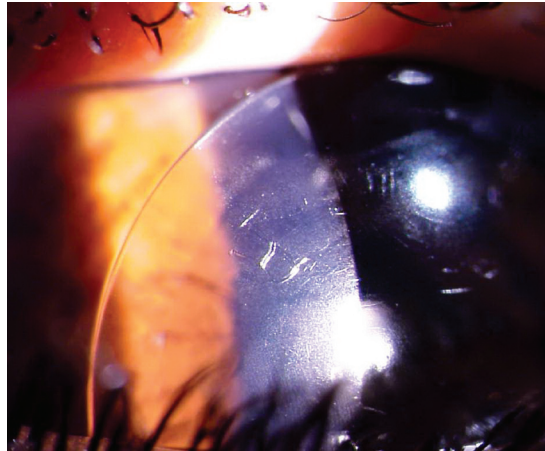


Figure 2
RGP with 'R' marking

power in the corneal plane of -4.75D, so this is the power we need for the contact lens.

The lens is 0.05mm steeper than K, so the liquid lens will have a power of +0.25D. To counter this we need to add -0.25D to the contact lens power, which takes us back to -5.00D. This is the power we will order.

If we decided that the 7.75 base curve looked a bit steep, we might decide to order a flatter lens next time. Suppose we wanted to order a BOZR of 7.85 this time. This is 2x0.05mm flatter than the previous lens, so we would create a tear lens with an extra -0.50D. We would need to modify the power of the lens we ordered by +0.50, so we would order -4.50D.

On the other hand, we might not do this, even if it is theoretically indicated, as we also need to consider the inconvenient fact that most of our patients have two eyes. These two eyes usually work together, though sometimes not as well as we might hope.

Binocular considerations

Myopes are likely to be exophoric, particularly at near fixation distances. If they wear their spectacles for near visual tasks, they will benefit from a certain amount of base-in prism at near, as the spectacles will be centred for distance. The loss of this base-in prism may result in decompensation of their near muscle balance, variable vision, asthenopic symptoms or even diplopia. In such cases, a slight over-correction of their myopia can sometimes be beneficial, as the extra accommodation stimulated will also induce accommodative convergence. With a normal accommodative convergence/accommodation (AC/A) ratio of around 4 even -0.25D can significantly alter the muscle balance without overloading accommodation itself. Accommodative demand is

higher for a myope in contact lenses than it is in spectacles. If the patient habitually reads without spectacles, as many low myopes do, they may initially struggle to cope with the extra accommodative demand that correction of their myopia brings. For these patients, over-correction is not appropriate.

Hyperopic patients often find near vision easier with contact lenses, as their accommodative and convergence demands are less. Practitioners should also beware the hyperope with a significant latent element, as their latent element sometimes seems to become manifest shortly after contact lens fitting.

Markings

It used to be common to see lenses marked 'R' and 'L' (Figure 2) and some lenses have the BOZR and TD printed on them as well. This is wonderful when doing aftercare, especially if you didn't fit the patient. However, engravings do tend to assist the formation of deposits and they may weaken a lens mechanically. A spate of RGP lenses splitting in line with the vertical part of the R and L led to many labs adopting a simpler method of discrimination between the two, and most lenses now have only a small dot on one lens, usually the right one. One consequence of this is that many patients, particularly those in early presbyopia, have no idea which lens is which, and may turn up for aftercare with either lens in either eye, or two of the same.

Tints

Some standard lenses come with a handling tint, which is intended to assist the detection of dropped lenses. The concept works well when white bathroom suites are in fashion, but less so when the height of lavatorial elegance comes in avocado or tasteful beige. In any case the handling tint is rarely an option, generally a standard feature of a particular lens. Similarly, many lenses have an UV inhibitor incorporated in the lens polymer, and occasionally this is offered as an optional extra. The ACLM manual identifies those lenses with an UV inhibitor. UV filtration may have long-term benefits for ocular health, particularly for those working outside, and aphakes. On the other hand, you should not attempt to examine the fluorescein pattern of a lens with a UV inhibitor with a Burton lamp. The cobalt blue light on a slit lamp will give a truer picture on these lenses.



CET Contact Lens Monthly

Summary

To order empirically, or to select from a trial set.

For a cornea with low toricity:

- TD should be large (approx 9.60mm) unless there are good reasons not to
- BOZD should be the same as flattest K or slightly flatter. Keratometers vary due to their different mire separation so get to know your instrument and allow for it
- Edge lift should be standard unless you know the patient isn't
- The lens edge needs to be 'well-rounded' or to have a well rounded front edge
- Centre thickness standard unless you are fitting a spherical lens on a cornea with significant astigmatism. In this case add 0.02 to the standard thickness. Manufacturers will usually allow for the flexibility of the lens material in setting their standard thickness
- Power should be the spectacle correction adjusted for vertex distance and the tear lens, unless you are trying something clever to help muscle balance. ●

● **Ngairé Franklin and Andy Franklin** are contact lens specialist optometrists practising in the South West

MULTIPLE-CHOICE QUESTIONS - take part at opticianonline.net

1 Which of the following is not an advantage of an alignment fit?

- A The lens weight is distributed over a maximum area
- B There is increased lens flexure enhancing tear exchange
- C There may be better tear exchange
- D Visual performance should be more stable

2 Which of the following is the best approach to fitting lenses of diameter greater than 9.50mm?

- A Fit on flattest K
- B Fit on steepest K
- C Fit just steeper than flattest K
- D Fit just flatter than flattest K

3 Which of the following most closely represents the band of fluorescein one may see around the edge of an RGP lens *in situ*?

- A Radial edge lift
- B Axial edge lift
- C Edge clearance
- D Peripheral optic zone radius

4 How is the flexure of an RGP lens related to the Dk?

- A No relationship
- B Increases with Dk
- C Decreases with Dk
- D Inverse square relationship

5 Which of the following represents the minimum thickness (in mm) recommended for a -4.00DS RGP lens?

- A 0.18
- B 0.16
- C 0.15
- D 0.14

6 For every 0.05mm that the BZOR is steeper than K, by how much does the power of the tear lens change?

- A -0.25D
- B +0.25D
- C -0.50D
- D +0.50D

Successful participation counts as one credit towards the GOC CET scheme administered by Vantage and one towards the Association of Optometrists Ireland's scheme. **The deadline for responses is July 29 2010**

One national contract shall be awarded on the basis of the most economically advantageous tender which offers high quality provision to meet the diverse needs of our customers and the Department.

A contract will be awarded for a period of 3 years with an option to extend for a further 2 years.

Initially this contract will only be used by DWP but the contract may be made available to other Government Departments. DWP estimate the overall contract value of between £1.7m and £3.8m, with an annual value following initial transition of between £21k and £140k.

Interested organisations are invited to visit the Supplying DWP website to view the specification and download a Pre-Qualification Questionnaire. Those organisations that are successful at PQQ stage will then be invited to submit a tender.

The deadline for return of PQQs is noon on 16th July 2010. Further details of how to return the PQQ can be found in the PQQ document.

Any queries please email the Project at DWP.OPTOMETRIST@DWP.PGSI.GOV.UK

Provision of Eye Care Specialist Reports

Following a change in legislation which will allow for prescribed categories of severely visually impaired people to be entitled to the Higher Rate Mobility Component (HRMC) of Disability Living Allowance (DLA) the Department for Work and Pensions is seeking to contract with a single supplier with local provision across the UK and including Northern Ireland, to undertake an examination of customers visual acuity and visual field, and provide a report back to The Department.

We will require the eye care specialist to:

- Undertake an examination and provide a report giving details of the customer's visual acuity measured by reference to the Snellen scale
- Provide the Department with a completed report and visual field charts to an agreed standard and in an agreed timescale.
- Have relevant equipment to perform an Esterman field test and undertake this to an agreed standard
- Make payment of reasonable customer expenses for attending if required by the Department.
- Be qualified and certified by a relevant government body.

DWP Department for Work and Pensions